



Cantilever anemometer based on a superconducting micro-resonator: Application to superfluid turbulence

J. Salort,^{a)} A. Monfardini, and P.-E. Roche
Institut Néel, CNRS/UJF BP 166, 38042 Grenoble cedex 9, France

(Received 26 October 2012; accepted 20 November 2012; published online 14 December 2012)

We present a new type of cryogenic local velocity probe that operates in liquid helium ($1\text{ K} < T < 4.2\text{ K}$) and achieves a spatial resolution of $\approx 0.1\text{ mm}$. The operating principle is based on the deflection of a micro-machined silicon cantilever which reflects the local fluid velocity. Deflection is probed using a superconducting niobium micro-resonator sputtered on the sensor and used as a strain gauge. We present the working principle and the design of the probe, as well as calibration measurements and velocity spectra obtained in a turbulent helium flow above and below the superfluid transition. © 2012 American Institute of Physics. [<http://dx.doi.org/10.1063/1.4770119>]

I. INTRODUCTION

Cryogenic helium is a fluid of high interest for hydrodynamics experiments because the control parameters (e.g., Reynolds number, Rayleigh number, etc.) can be varied over decades and can reach much higher values than most room temperature laboratory experiments.¹⁻⁵ One of the main challenges for the experimentalist is then to come up with fast micro-sensors suited to helium flows. Over the last two decades, there has been various developments of local cryogenic probes, specifically hot wires,^{2,6,7} micro-thermometers,^{8,9} second-sound tweezers,¹⁰ Pitot-tube-like anemometers,^{11,12} vibrating wires,^{13,14} and quartz tuning forks.^{15,16}

When liquid helium is cooled below $T_\lambda \approx 2.17\text{ K}$ (at saturated vapor pressure), it undergoes a phase transition. The classical phase, above T_λ , is called He I. It is a classical fluid with finite viscosity. The phase obtained for temperature below T_λ , is called He II. It can be described by the so-called two-fluid model, i.e., as a superposition of a normal component which behaves like a classical fluid (finite viscosity) and a superfluid one with zero-viscosity and quantized vorticity.¹⁷

The smallest, fastest, and most widely used local anemometers in turbulence studies are hot-wires. However it is not straightforward to use these probes below the superfluid transition. Indeed, heat is transported very efficiently in the bulk of liquid He II by propagating temperature waves^{18,19} and the temperature is roughly homogeneous. While this property of efficient heat transport has proven useful for applications of superfluid helium as a coolant (for example to cool large superconducting coils²⁰), it is a major pitfall for temperature-sensitive probes such as hot-wires. So far, the best replacement for velocity measurements has been miniature Pitot tubes produced from cryogenic pressure transducers using dedicated nozzles with external diameters down to 0.6 mm .¹² Yet for turbulence applications, where smaller probes are needed to resolve the dissipative scales,

this approach seems to have nearly reached its limit. Indeed, while the probing of smaller scales requires higher sensibility (smaller eddies are less energetic), reducing the size of a pressure transducer means reducing the diameter of the sensitive membrane and therefore its sensitivity. The alternative method presented in this paper consists in replacing the sensitive membrane by a cantilevered beam. Since it is anchored at only one end, the deflection for a given load is larger than for a membrane of the same size. This leads to higher sensitivity and enable further miniaturization. Other advantages of this type of probes over hot-wires or Pitot tubes are that it measures velocity magnitude and direction and is more immune to acoustic noise than Pitot tubes.²¹ Additionally, the time response of Pitot tubes is limited by a dead volume of fluid. Cantilevers do not suffer from this drawback.

This cantilever-sensing approach has long proven fruitful for atomic force microscopy. More recently, Barth *et al.* demonstrated the use of cantilevers as accurate anemometers for room-temperature turbulence measurements in air and water.^{22,23} This room-temperature cantilever anemometer uses optical means to accurately measure the beam deflection. This optical approach cannot be brought to cryogenic environment easily. Instead, we present an original method to measure fast fluctuations of the strain on the beam. It is based on a recent technological breakthrough originally aimed at cosmic particles detection and high sensitivity millimeter-wave imaging of the cosmic microwave background.

There is a number of cryogenic hydrodynamic problems that may benefit from this kind of anemometer. (i) The understanding of superfluid turbulence suffers from the lack of spatially-resolved fluctuation data.¹⁷ (ii) In thermal convection, hot-wire measurements are biased by thermal plumes. A reliable local anemometer is still lacking. (iii) The boundary layer thickness in turbulent helium flows is usually small, smaller than $100\text{ }\mu\text{m}$ in most cases. Therefore smaller probes are necessary to study it.

The aim of this paper is to discuss the working principle, the details of the construction and driving electronics of a cantilever anemometer specifically designed for superfluid helium.

^{a)}Present address: Laboratoire de physique, ENS Lyon - 46 allée d'Italie - 69364 Lyon cedex 7, France.

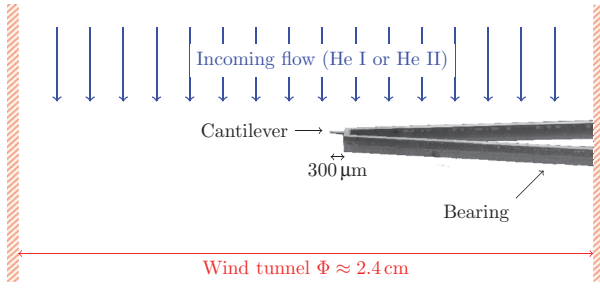


FIG. 1. Cantilever anemometer in the bulk of a liquid helium flow.

II. WORKING PRINCIPLE

The sensitive part of this anemometer is a $100 \mu\text{m} \times 300 \mu\text{m}$ silicon cantilever of thickness between $1 \mu\text{m}$ at the tip and $10 \mu\text{m}$ near the base. A measurement of the strain induced by the incoming flow on this cantilever leads to an estimate of the local velocity (see Figure 1). If the fluid comes from the opposite direction, the load is applied on the opposite side of the cantilever: a strain measurement therefore allows an estimate for the velocity magnitude and direction. The deflection s can be estimated using the same hypothesis as in the room temperature case,²²

$$s = \text{sign}(v) \frac{\ell^3}{8} \frac{P \ell w}{EI}, \quad (1)$$

where $\text{sign}(v) = \pm 1$ depending on the flow direction, ℓ is the length on the beam, w its width, e its thickness, P is the applied uniform pressure due to the incoming flow, E is the Young modulus of silicon (its value spans from 130 GPa to 170 GPa depending on the crystal axis, it does not change significantly when the temperature is decreased) and $I = \frac{1}{12} w e^3$ is the inertial momentum. Our probe is sensitive to the relative elongation (or relative contraction if $v < 0$) of the upper surface, that can be derived from Eq. (1),

$$\frac{\Delta \ell}{\ell} \sim \text{sign}(v) \frac{P \ell^2}{E e^2}. \quad (2)$$

The pressure load on the beam due to the flow can be estimated as,

$$P = \frac{1}{2} c_d(v) \rho v^2, \quad (3)$$

where $c_d(v)$ is the drag coefficient and $\rho \simeq 145 \text{ kg/m}^3$ the fluid density. Above the superfluid transition, the typical Reynolds number of the probe, $Re_\ell = \ell \langle v \rangle / \nu \approx 100$ to 10^4 in the velocity range $\langle v \rangle \approx 0.01 \text{ m/s}$ to 1 m/s . Therefore, the classical drag coefficient, c_d is of order 1 and nearly constant.²⁴ Experiments suggest that drag forces in turbulent superfluid helium are similar to those in the classical case.^{16,25,26} Therefore, it seems reasonable to take $c_d(v) = O(1)$ to compute a rough estimate of the relative elongation, here for $\langle v \rangle = 1 \text{ m/s}$,

$$\frac{\Delta \ell}{\ell} \approx 5 \times 10^{-5}. \quad (4)$$

This relative elongation is rather small and therefore always in the linear regime.

To perform fast and sensitive measurements of the deflection of the beam, an accurate strain gauge is needed. Our detection method is based on a superconducting micro-resonator. This technology was initially aimed at astrophysics applications.^{27–29} It consists in a lumped-element high-quality-factor radio-frequency micro-resonator patterned in a thin superconducting layer^{30,31} sputter-deposited on the silicon substrate. In the case of astrophysics detectors, absorbed particles (cosmic particles or microwave photons) lead to the breaking of Cooper-pairs and thus to a shift in the resonator kinetic inductance³² and therefore to a measurable shift of its resonance frequency.

In this work, we demonstrate another possible use of this highly sensitive resonators as strain gauge. The resonator geometry and the superconducting material (200 nm-thick sputter-deposited niobium layer) are chosen such that the kinetic inductance is much lower than the geometric inductance, so that unavoidable cosmic particles do not produce spurious noise. The lumped-element radio frequency circuit consists in a LC pattern in which the inductance and the capacitance parts are separated. The inductance is obtained with a meandering pattern, placed on the probe Si chip but outside the flow. This part of the impedance does not depend on the flow velocity. The capacitance originates from inter-digitated fingers located on the cantilevered beam. This part of the impedance is modified when the beam gets elongated. The full niobium pattern is shown in Figure 2. As a consequence, the relative elongation of the cantilever is designed to result in a measurable shift in resonance frequency.

III. DESIGN AND OPERATION

The micro-device — cantilever and bearing arms — is patterned from a $350 \mu\text{m}$ -thick (100) silicon wafer with double-side photolithography and subsequent deep-reactive-ion-etching (DRIE) in $\text{SF}_6/\text{O}_2/\text{C}_4\text{F}_8$ plasma (Bosch process). This lets us choose the geometry of both the sensitive part and the bearing arms to make them rigid and as little invasive as possible for the incoming flow. There are two arms to ensure lateral rigidity. The double side mask is realized with a 400 nm evaporated aluminum layer. This aluminum is removed at the end of the machining process with a $\text{H}_3\text{PO}_4/\text{CH}_3\text{CO}_2\text{H}/\text{H}_2\text{SO}_4$ liquid mixture.

The use of a barrier layer — SiO_2 or Si_3N_4 typically — to control the thickness of the cantilever had to be avoided because the presence of an amorphous dielectric layer is known to produce unwanted spurious frequency and phase noise on superconducting resonators.^{33,34} It is then a technical challenge to leave a $1 \mu\text{m}$ -thick cantilever from a $350 \mu\text{m}$ bulk silicon substrate. However, one advantage is that the obtained cantilever is made of mono-crystalline silicon and thus does not hold residual stresses.

To solve this problem, we etched $1 \mu\text{m}$ -deep holes in the wafer top side beforehand (see Figure 3). This leads to a detectable leak between both sides of the wafer during the etching process. When the cantilever tip, being etched from the bottom side, reaches its desired thickness, the gaseous helium cooling jet leaks into the DRIE plasma chamber, which is detected by the pressure regulation systems. The

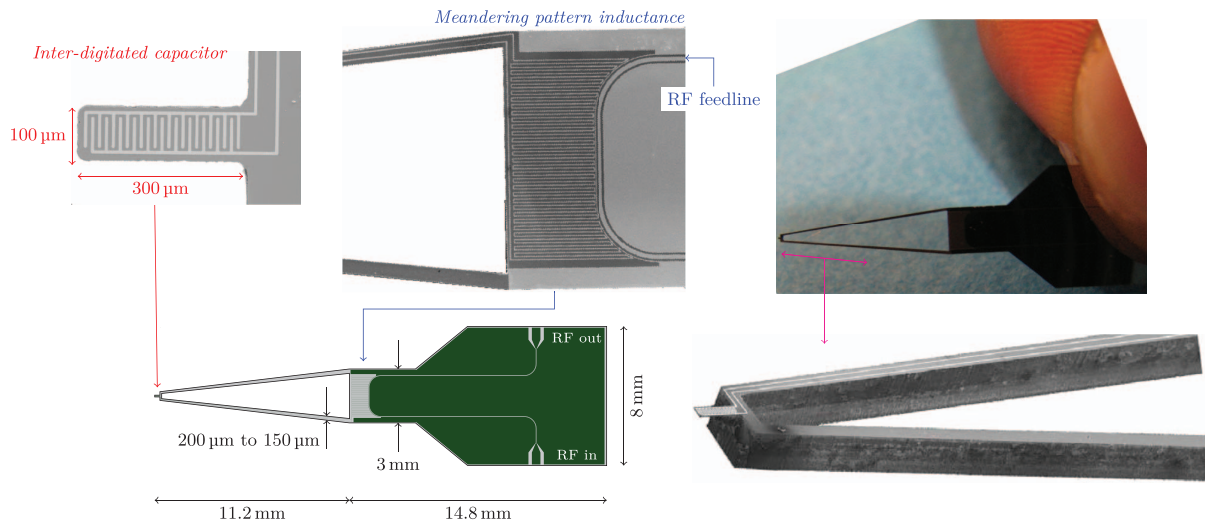


FIG. 2. Main dimensions of the probe and niobium pattern of the micro-resonator circuit. The three grayscale images are SEM pictures.

actual cantilever thickness can be estimated from SEM pictures such as the one shown in Figure 2 by counting the alternating black and white stripes (called “scallop”) on the cantilever side. These are due to the Bosch process alternating cycles. Each cycle roughly etches 1 μm in the silicon substrate. The obtained cantilever is slightly less than 1 μm at its tip and close to 10 μm close to the anchor. This inhomogeneity helps to concentrate the sensitivity to the flow velocity on the tip of the cantilever.

The superconducting micro-resonator is patterned on a 200 nm niobium layer sputter deposited on the silicon substrate. We use UV-photolithography and subsequent reactive-ion etching in a SF₆/O₂ plasma. Niobium was chosen for its ease of use and its relatively high T_c of ~ 9 K.

The micro-resonator is coupled to a coplanar waveguide, called “RF feedline.” To sense the resonance frequency of the resonator, a microwave is sent in this waveguide at the port labeled “RF in” and probed at the exit at the port labeled “RF out” (see Figure 2). A microwave power between -30 dBm

and -20 dBm was chosen to get as much output power as possible without weakening the resonance. When the wave frequency matches the LC resonance frequency, part of its energy is transferred to the resonator and the amplitude of the transmitted wave decreases. The coplanar waveguide can be described by a transfer matrix S . In the following, we only measure and discuss the transmission function, $|S_{21}|$, where 2 represents the “RF out” port and 1 the “RF in” port. This function reaches a minimum when the input wave frequency matches the LC resonance frequency, around 1 GHz in our case.

The absorption peak is shown in Figure 4. The coupling strength, and thus the resonance features (depth and width)

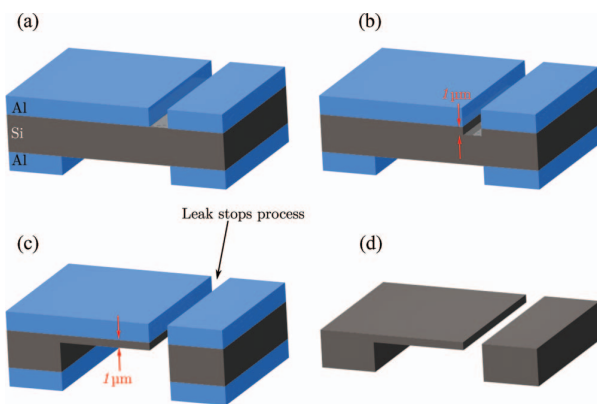


FIG. 3. Schematic description of the deep-etching steps. (a) Bulk silicon wafer with aluminum masks on both sides. (b) 1 μm-deep RIE etching of top side. (c) Deep-etching of bottom side until a leak is detected. (d) Final structure after cleaning the aluminum layers.

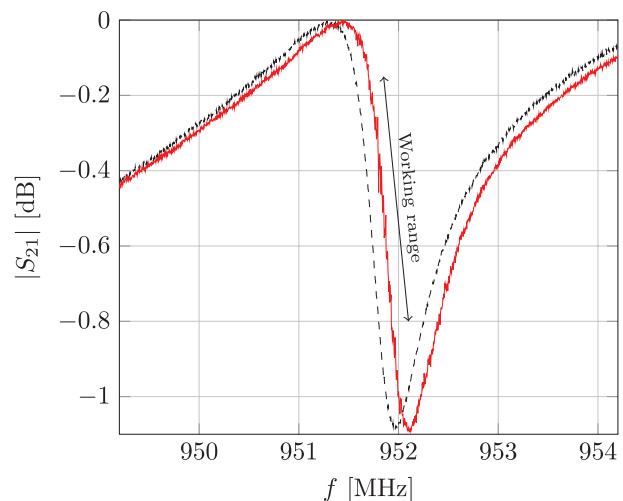


FIG. 4. Transmission coefficient S_{21} through the superconducting feedline (see text) measured with a Vector Network Analyser at $T = 1.67$ K. The input power on the feedline is -20 dBm. The resonance frequency of this LC-resonator is 952 MHz. The quality factor is $Q \approx 10^3$. The fluid mean velocity is either zero (black dashed line) or ≈ 1 m/s (red line). The “working range” corresponds to the frequency range in which the carrier frequency is chosen when the resonator is probed by frequency modulation (see Figure 5).

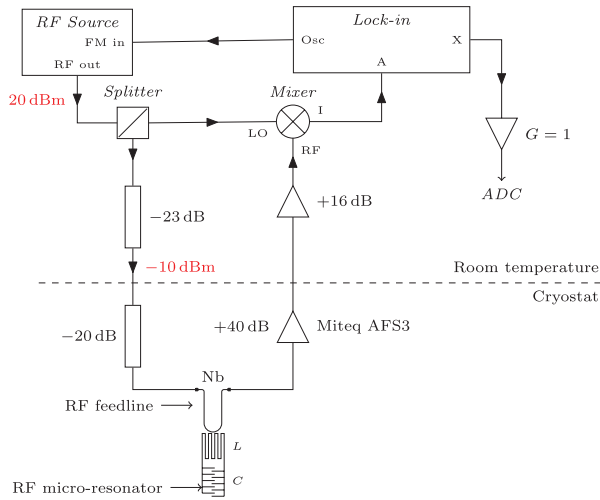


FIG. 5. Electronic diagram used to perform the fluctuations measurements of the cantilever elongation by frequency modulation.

can be tuned by adjusting the distance between the 50 Ω -coplanar waveguide and the meandering pattern inductance (in our case, 18 μm overall). The observed resonance is asymmetrical, probably because of the parasitic inductance of the aluminum bondwires, known to be enhanced when the coupling between the feedline and the resonator is strong.³⁰ The quality factor is large enough for the present application. Yet, it is relatively weak — around 1 dB deep. The most likely reason is the presence of residual traces of aluminum, passivated by the high-power fluoride plasma during the DRIE steps. Their presence on the niobium circuit has been confirmed by energy-dispersive X-ray spectroscopy analysis. Therefore, it is possible to improve the probe sensitivity further if additional cleaning steps are devised to remove those spurious traces of aluminum.

A measurement consists in evaluating the transmission S_{21} at a given frequency, close to the absorption peak. When the cantilever gets deflected because of the incoming flow, the LC resonance frequency is modified and the output power changes (as illustrated in Figure 4). To probe velocity fluctuations, dynamic measurements of the amplitude $|S_{21}(t)|$ have to be carried out.³⁵ To do this with a large signal-to-noise ratio, we use a frequency modulation (FM) measurement technique. The FM wave is sent in the niobium coplanar waveguide. The output wave is amplified at low-temperature with a low-noise cryogenic RF amplifier (Miteq AFS3) located in the vapor of the helium bath of the cryostat, on its lowest thermal screen (the amplifier's casing temperature is close to the liquid helium bath temperature) and recombined with the initial wave using a mixer at room temperature. The amplitude-modulated signal is then demodulated with a lock-in amplifier. The full electronic diagram is shown in Figure 5.

IV. IN-FLOW VALIDATION

The probe, shown in Figure 2, was placed in a cryogenic wind tunnel. It consists a He II loop continuously powered by a centrifugal pump. Turbulence is probed in a $\Phi = 23$ mm diameter, 250 mm long stainless steel pipe, located upstream

the pump. On the return path and at the entrance of the pipe, honeycombs break the spin motion generated by the pump. This cryostat was described in more details in a previous paper.¹⁰

In the present flow setup, we have added a centered 2.0 mm-thick brass disc with diameter $\varnothing_d = 11$ mm at the entrance of the pipe which acts as wake generator. The cantilever probe is located 10 cm downstream from the disc. This disc has the same proportions as the one we used recently in a far-wake superfluid turbulent flow experiment in a larger wind tunnel,³⁶ which showed that the Strouhal number, in such a configuration,

$$St = \frac{f_0 \varnothing_d}{\langle v \rangle} \quad (5)$$

is similar above and below the superfluid transition, where f_0 is the frequency of the observed vortex shedding and $\langle v \rangle$ is the flow velocity average over the pipe section.

The mean velocity in the wind tunnel can be varied up to 1.35 m/s, corresponding to a Reynolds number based on the Taylor microscale $R_\lambda \approx 1000$ in He I. The temperature can be varied above and below the superfluid transition at ≈ 2.17 K. The turbulence is probed in the far-wake of the disc.

The cantilever probe is calibrated against a miniature Pitot probe, at several temperatures. The raw data points in He II are shown in Figure 6 for temperature from 1.66 K to 2.07 K, which corresponds to concentration of superfluid component, ρ_s/ρ , ranging from 80% to 30%, respectively. At each temperature, the calibration dataset is obtained by stepwise increase and decrease of the rotation speed of the wind-tunnel propeller. Each step includes a 20-s pause allowing the hydrodynamical and thermal transient behaviours to relax, followed by a 3-s averaging of the cantilever probe signal. The scatter in the calibration plot (see Figure 6) is interpreted as the result of the fluctuations in the wind-tunnel

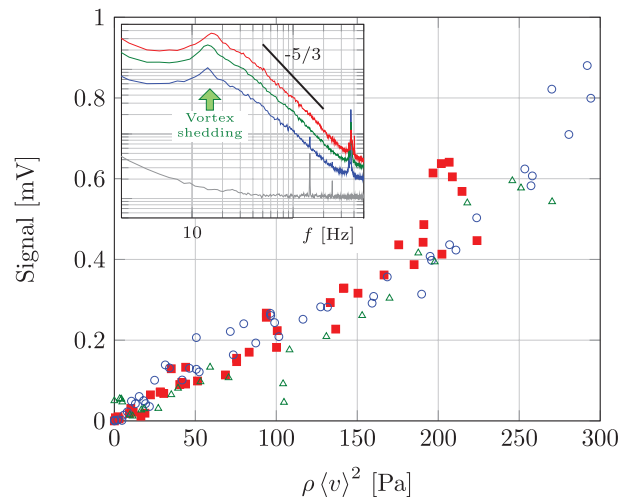


FIG. 6. Calibration of the probe in He II. Open green triangles: $T = 2.07$ K ($\rho = 145.8$ kg/m³). Red squares: $T = 1.82$ K ($\rho = 145.4$ kg/m³). Open blue circles: $T = 1.66$ K ($\rho = 145.3$ kg/m³). Insert: Power spectra of the fluctuating signal. From bottom up: 0 m/s and 1 m/s at $T = 1.66$ K, 1.1 m/s and 1.35 m/s at $T = 1.82$ K. The green arrow points toward the vortex shedding peak.

(residual transient motions and turbulent fluctuations) and not to the intrinsic noise of the probe, nor from electronic noises. Two types of measurements support this interpretation. First, the intrinsic noise of the electronics is measured in quiescent superfluid helium. The spectral density of the corresponding noise signal, plotted in the insert of Figure 6 (lower curve), is significantly lower than the spectral density of the signal in presence of a flow. The second test — presented in the next paragraph — consists in comparing the fluctuations spectra measured by the cantilever probe with the expected turbulent velocity spectra. The calibration in He I was more difficult because of the sporadic presence of bubbles in this specific wind tunnel. We find that the obtained signal scales like $\rho \langle v \rangle^2$ to a good approximation and do not seem to depend on temperature, as expected (see Eqs. (2) and (3)).

The power spectra of the signal, obtained for several superfluid turbulent conditions, are shown in insert of Figure 6. They exhibit expected hydrodynamic features:³⁶ (i) a low frequency plateau up to 20 Hz corresponding to scales larger than the injection scale, (ii) a vortex shedding peak near 15 Hz and (iii) nearly a decade of $f^{-5/3}$ Kolmogorov scaling corresponding to inertial scales of the turbulent cascade.

V. CONCLUSION AND PERSPECTIVES

We have realized and operated the first cantilever anemometer dedicated to cryogenic turbulence and the first fully micromachined local probe for cryogenic hydrodynamics. The calibration and turbulent fluctuations measurements validate the principle of cantilever anemometry for superfluid flows. This technology improves the spatial resolution by a factor of 10 compared to the best alternative anemometers known to work in superfluid helium.

The cantilever approach has several advantages over traditional pressure-transducer based anemometers and supersedes Pitot tube probes in many aspects: (i) it is fully micromachined, which opens the way to further miniaturization down to scales where quantum effects are supposedly occurring in superfluid turbulence at finite temperature,³⁶ (ii) it is mostly immune to acoustic perturbations which is one of the main noise sources in high-Reynolds number superfluid wind tunnels, (iii) it provides the sign of the velocity, and (iv) the spurious heat dissipation is negligible thanks to the superconducting technology (below 1 μ W). This is a major advantage for thermal convection systems.

This work also demonstrates the interest and efficiency of superconducting micro-resonators for fine hydrodynamic measurements. Since the resonance frequency depends on the dielectric permittivity of the fluid³¹ and therefore on the local density (and $\rho(T) \propto T$), this opens the way to other possible use in cryogenic turbulence, such as local density or temperature measurements. Additionally, it was shown previously that large numbers of these micro-resonators can be multiplexed on a single feedline,²⁹ which allows to build arrays of cantilevers and therefore grants access to spatial velocity correlations. These multiplexed superconducting resonators can also be deposited on a surface to obtain an image of its temperature. One may think for example to realize thermal imaging of the boundary layer in cryogenic convection experiments

where the heat flux spatial behavior is an important open question directly related to the ultimate regime of convection.^{37,38}

ACKNOWLEDGMENTS

This work was performed with the help of “Plateforme Technologie Amont” (PTA) in Grenoble and with financial support of the ANR (Grant Nos. “SHREK” ANR-09-BLAN-0094 and “MKIDS” ANR-09-JCJC-0021-01). We are grateful to T. Haccart, S. Litaudon, F. Gustavo, C. Lemonias and J.-L. Thomassin for their expertise in the clean room. We thank G. Garde for his availability and skills on the cryogenic apparatus, and C. Thirion, C. Hoarau, V. Bouchiat, and B. Hébral for many stimulating discussions.

- ¹O. Chanal, B. Chabaud, B. Castaing, and B. Hébral, *Eur. Phys. J. B* **17**, 309 (2000).
- ²S. Pietropinto, C. Poulain, C. Baudet, B. Castaing, B. Chabaud, Y. Gagne, B. Hébral, Y. Ladam, P. Lebrun, O. Pirotte, and P. Roche, *Physica C* **386**, 512 (2003).
- ³P.-E. Roche, F. Gauthier, R. Kaiser, and J. Salort, *New J. Phys.* **12**, 085014 (2010).
- ⁴J. J. Niemela, L. Skrbek, K. R. Sreenivasan, and R. J. Donnelly, *Nature (London)* **404**, 837 (2000).
- ⁵P. Urban, P. Hanzelka, T. Kralik, V. Musilova, L. Skrbek, and A. Srnka, *Rev. Sci. Instrum.* **81**, 085103 (2010).
- ⁶B. Castaing, B. Chabaud, and B. Hébral, *Rev. Sci. Instrum.* **63**, 4167 (1992).
- ⁷J. Maurer, P. Tabeling, and G. Zocchi, *EPL* **26**, 31 (1994).
- ⁸O. Chanal, B. Bagueard, O. Béthoux, and B. Chabaud, *Rev. Sci. Instrum.* **68**, 2442 (1997).
- ⁹F. Gauthier, J. Salort, O. Bourgeois, J.-L. Garden, R. du Puits, A. Thess, and P.-E. Roche, *EPL* **87**, 44006 (2009).
- ¹⁰P.-E. Roche, P. Diribarne, T. Didelot, O. Français, L. Rousseau, and H. Willaime, *EPL* **77**, 66002 (2007).
- ¹¹J. Maurer and P. Tabeling, *EPL* **43**, 29 (1998).
- ¹²J. Salort, P. Diribarne, B. Rousset, Y. Gagne, B. Dubrulle, T. Didelot, B. Chabaud, F. Gauthier, B. Castaing, and P.-E. Roche, *Phys. Fluids* **22**, 125102 (2010).
- ¹³D. I. Bradley, D. O. Clubb, S. N. Fisher, A. M. Guénault, R. P. Haley, C. J. Matthews, G. R. Pickett, and K. L. Zaki, *J. Low Temp. Phys.* **138**, 493 (2005).
- ¹⁴Y. Nago, T. Ogawa, K. Obara, H. Yano, O. Ishikawa, and T. Hata, *J. Low Temp. Phys.* **162**, 322 (2011).
- ¹⁵R. Blaauwgeers, M. Blažková, M. Človečko, V. B. Eltsov, R. de Graaf, J. Hosio, M. Krusius, D. Schmoranzler, W. Schoepe, L. Skrbek, P. Skyba, R. E. Solntsev, and D. E. Zmeev, *J. Low Temp. Phys.* **146**, 537–562 (2007).
- ¹⁶D. Schmoranzler, M. L. Mantia, and L. Skrbek, *EPJ Web Conf.* **25**, 02025 (2012).
- ¹⁷L. Skrbek and K. R. Sreenivasan, *Phys. Fluids* **24**, 011301 (2012).
- ¹⁸L. Landau, *Phys. Rev.* **60**, 356 (1941).
- ¹⁹S. V. Sciver, *Helium Cryogenics* (Springer, 1986).
- ²⁰P. Lebrun and L. Tavian, in *Proceedings of CAS - CERN Accelerator School on Superconductivity and Cryogenics for Accelerators and Detectors* (CERN, 2002), pp. 375–389.
- ²¹An acoustic perturbation would be sensed equally by both sides, at first order.
- ²²S. Barth, H. Koch, A. Kittel, J. Peinke, J. Burgold, and H. Wurmus, *Rev. Sci. Instrum.* **76**, 075110 (2005).
- ²³M. Hölling and J. Peinke, *Springer Proc. Phys.* **131**, 61 (2009).
- ²⁴R. L. C. Flemmer and C. L. Banks, *Powder Technol.* **48**, 217 (1986).
- ²⁵M. R. Smith, D. K. Hilton, and S. W. V. Sciver, *Phys. Fluids* **11**, 751 (1999).
- ²⁶M. Blažková, D. Schmoranzler, and L. Skrbek, *Phys. Rev. E* **75**, 025302(R) (2007).
- ²⁷P. K. Day, H. G. LeDuc, B. A. Mazin, A. Vayonakis, and J. Zmuidzinas, *Nature (London)* **425**, 817 (2003).
- ²⁸B. A. Mazin, “Microwave kinetic inductance detectors,” Ph.D. dissertation, California Institute of Technology, 2004.
- ²⁹A. Monfardini, L. Swenson, A. Bideaud, F. Désert, S. Yates, A. Benoit, A. Baryshev, J. Baselmans, S. Doyle, B. Klein, M. Roesch, C. Tucker, P. Ade,

- M. Calvo, P. Camus, C. Giordano, R. Guesten, C. Hoffmann, S. Leclercq, P. Mauskopf, and K. Schuster, *Astron. Astrophys.* **521**, A29 (2010).
- ³⁰S. Doyle, P. Mauskopf, J. Naylon, A. Porsch, and C. Duncombe, *J. Low Temp. Phys.* **151**, 530 (2008).
- ³¹G. Grabovskij, L. Swenson, O. Buisson, C. Hoffmann, A. Monfardini, and J.-C. Villégier, *Appl. Phys. Lett.* **93**, 134102 (2008).
- ³²The inertia of the superconducting, lossless charge carriers, i.e., the Cooper pairs, leads to an equivalent inductance term called “kinetic inductance,” e.g., see V. V. Schmidt, *The Physics of Superconductors* (Springer, Berlin, 1997).
- ³³S. Kumar, J. Gao, J. Zmuidzinas, B. A. Mazin, H. G. LeDuc, and P. K. Day, *Appl. Phys. Lett.* **92**, 123503 (2008).
- ³⁴R. Barends, H. L. Hortensius, T. Zijlstra, J. J. A. Baselmans, S. J. C. Yates, J. R. Gao, and T. M. Klapwijk, *Appl. Phys. Lett.* **92**, 223502 (2008).
- ³⁵An alternative approach is to measure the phase of S_{21} instead of its amplitude.
- ³⁶J. Salort, B. Chabaud, E. Lévêque, and P.-E. Roche, *EPL* **97**, 34006 (2012).
- ³⁷F. Gauthier and P.-E. Roche, *EPL* **83**, 24005 (2008).
- ³⁸F. Chillà and J. Schumacher, *Eur. Phys. J. E* **35**, 58 (2012).